

# BreezeSuite™ Cardiorespiratory Diagnostic Software

## Version 8.6

### Standalone Client Workstation Upgrade Manual



#### Contact

**MGC Diagnostics Corporation through its subsidiary Medical Graphics Corporation**

350 Oak Grove Parkway

St. Paul, Minnesota USA 55127-8599

T +1 651.484.4874

800.950.5597

F +651.484.8941



# CONTENTS

Introduction.....	3
Purpose of this Manual.....	3
The Upgrade Process .....	3
Professional Installation Service .....	3
System Specification: Client.....	4
Required Operating System .....	4
Processor .....	4
Hard Disk.....	4
Memory .....	4
Display .....	4
System Type.....	4
Other Hardware.....	4
System security considerations .....	5
Data at Rest Encryption .....	5
Data at Rest Prevention.....	5
Data in Transit Encryption .....	5
SQL Database Connection Information Encrypted .....	5
SQL Database Naming .....	5
Authentication in SQL Server.....	5
Authentication in BreezeSuite v8.6 .....	6
Antivirus and Anti-Malware Software Policy .....	6
Operating System Update Policy .....	6
Pre Installation requirements .....	7
Update the Operating System .....	7
Windows Administrator Permissions Required for Installation .....	7
Computer Naming Considerations.....	7
Prevent Windows Users from Changing Date, Time and Time Zone .....	8
Post Installation requirements .....	9
Required Windows User Rights (Permissions) .....	9
BreezeSuite v8.6 Standalone Client UPGRADE .....	122
BreezeSuite Software License Agreement.....	177

# INTRODUCTION

## Purpose of this Manual

This manual provides instructions on how to upgrade your BreezeSuite™ cardiorespiratory diagnostic software to BreezeSuite v8.6.

## The Upgrade Process

Obtain all of the required resources before upgrade. These include:

- A copy of the BreezeSuite v8.6 software media
- Appropriate Windows Administrator user credentials for the client workstation computer
- Your facilities policies regarding use and configuration of SQL Server Express configuration

## Professional Installation Service

MGCD Diagnostics offers professional installation and upgrade service (service fees apply).

Professional service installation benefits include:


- Remote or onsite installation service
- Scheduled and reliable software installation for minimal downtime
- Software configuration assistance
- Report customization assistance
- Predicted set configuration assistance
- Diagnostics testing screen customization assistance
- Application security configuration guidance
- Data conversion assistance
- Device communication verification

Please contact MGC Diagnostics to discuss the installation service options available.

Phone: 800-333-4137

Email: [Support@MGCDiagnostics.com](mailto:Support@MGCDiagnostics.com)

## SYSTEM SPECIFICATION: CLIENT

Required Operating System	Windows 11 (Pro or Enterprise) Windows 10 (Pro, Enterprise or Enterprise LTSB) Windows 8.1 (Pro or Enterprise) Windows 7 (Pro, Ultimate or Enterprise) Service Pack 1  <b>Note:</b> Windows 7 support ended January 2020
Processor	Intel Core Duo or Greater
Hard Disk	80+ GB Recommended
Memory	8+ GB Recommended
Display	1024 x 768 Resolution Minimum
System Type	x64 (64-Bit) Recommended X84 (32-Bit) Supported
Other Hardware	3+ USB-A Ports (if client connecting to diagnostic device)

# SYSTEM SECURITY CONSIDERATIONS

## Data at Rest Encryption

BreezeSuite 8.6 software supports the use of commercial off the shelf (COTS) Full Disk Encryption technology including Bitlocker configured for Federal Information Processing Standards (FIPS) Publication 140-2 compliance.

## Data at Rest Prevention

BreezeSuite 8.6 software, when installed and connected to a Network SQL Database, supports installation without a local SQL Database. This new feature ensure no ePHI data at rest and removes the need to maintain SQL Server Express updates and patches. MGC Diagnostics recommends using this feature on all network clients where reliance on a local database mode is not required. This feature should be used on all networked physician review BreezeSuite installations as physician review can only be performed when connected to the network database.

## Data in Transit Encryption

BreezeSuite 8.6 software, when installed and connected to a Network SQL Database, supports use of TLS 1.2 encrypted SQL Server connections. MGC Diagnostics recommends configuring your Network SQL Server and client for TLS 1.2 encryption.

## SQL Database Connection Information Encrypted

BreezeSuite 8.6 software stores SQL database connection information in an encrypted file to prevent viewing by unauthorized users. Connection information can only be viewed by an authenticated user using the BreezeSuite DBTools application.

## SQL Database Naming

BreezeSuite 8.6 software supports customizing the name(s) of the BreezeSuite application SQL Databases. This allows for additional database security as well as allows for hosting both Test/Development and Production BreezeSuite databases within the same SQL Instance.

## Authentication in SQL Server

BreezeSuite 8.6 software supports use of Windows Authentication for BreezeSuite database SQL Logins/Users. MGC Diagnostics recommends using Windows authentication wherever possible.

BreezeSuite 8.6 software also supports the use of customized SQL Authentication usernames and passwords. MGC Diagnostics strongly recommends changing all default SQL Authentication user names and passwords to unique user names and strong customized passwords.

## Authentication in BreezeSuite v8.6


BreezeSuite 8.6 software supports use of Active Directory authentication for BreezeSuite application users. See the Security Administrators Guide for additional details and configuration information.

## Antivirus and Anti-Malware Software Policy

MGC Diagnostics has an open policy regarding customer's use of commercial off the shelf (COTS) antivirus and anti-malware software. Customers may install, update and patch anti-virus and anti-malware software without pre-approval from MGCD Diagnostics.

## Operating System Update Policy

MGC Diagnostics recommends applying Operating System updates and patches on a regular basis. MGC Diagnostics does not provide a release schedule or list of approved updates and recommends installing updates as they are made available from the computer hardware and operating system manufacturer.

 **Important:** If updates are checked, downloaded or installed during diagnostic testing, this may result in degraded system performance, software errors and data loss.

# PRE INSTALLATION REQUIREMENTS

## Update the Operating System

Verify all available Windows Service Packs, Updates and Patches have been installed

## Windows Administrator Permissions Required for Installation

Domain Administrator permission required when installing BreezeSuite on a client computer registered to the Network/Domain.

Local Windows Administrator permission required when installing BreezeSuite on a client computer not connected to a network/domain.

## Computer Naming Considerations

The BreezeSuite application registers system/workstation settings to the computer name. Whenever possible, perform computer name changes prior to BreezeSuite software installation to prevent loss of system/workstation settings in the application.

If replacing a computer due to hardware failure, renaming the new computer to the same computer name as the faulty computer will preserve the system/workstation settings in the application.

**ⓘ Important:** If a computer name change is required after installation on a system with the BreezeSuite local SQL Database feature installed, contact MGC Diagnostics technical support for guidance to avoid software down time.

**ⓘ Important:** Registering two or more active workstation computers with the same computer name to a BreezeSuite Network SQL Database will cause application issues. Unique computer names must be used for all active workstations when connected to a Network SQL Database.

When changing the computer name, updates to BreezeSuite registry keys will be required. By default, the local SQL Server name is the same as the local computer name.

BreezeSuite relies on DB Tools for database management. To update this, navigate to the Database Configuration screen located within DB Tools.

1. Prior to opening DB Tools, the BreezeSuite program must be closed.
2. Right Click on DB Tools and run the application as administrator.
3. Login to DB Tools using a BreezeSuite user name and password with the appropriate permissions.
4. Select the Admin tab and then select Database Configuration.
5. Confirm that the BreezeSuite database is not in use by selecting OK.
6. Update the local Server Name to reflect the updated computer name.

## Prevent Windows Users from Changing Date, Time, and Time Zone

Recommend that Date/Time controls within Windows are implemented to ensure data integrity of the audit log.

*Note: User must have administrator privileges.*

1. Open Local Security Settings:
  - i) Press the Windows key + R together to open the Run command. Type **secpol.msc** and hit Enter to open the Local Security Policy window.
  - ii) On the left-hand side, Select **Local Policies -> User Rights Assignment**.
  - iii) On the right, double-click the "**Change the system time**" setting to modify.
2. Allow or Disallow Administrator and Users
  - i) Highlight **Administrators** in the Change the system time Properties. Do NOT remove LOCAL SERVICE.
  - ii) Click the Remove button to disallow administrators to change the Date and Time.
3. Allow a specific administrator (instead of all administrators) to have exclusive access to date/time settings
  - i) In the Properties window, click on **Add User or Group**.
  - ii) Click on the **Advanced...** button.
  - iii) Click on the **Find Now** button.
  - iv) Select the name of the specific group that will be allowed to edit Date and Time.
  - v) Click **Apply** and then **OK**. Restart the computer for this policy to take effect.
4. Repeat Steps 1-3 with the exception of double-clicking on '**Change the time zone**' instead of '**Change the system time**' in step 1(iii)

# POST INSTALLATION REQUIREMENTS

## Required Windows User Rights (Permissions)

All BreezeSuite users must have their Security User Permissions set to 'Full control' for the following folders and all child objects:

- C:\Program Files (x86)\Medgraphics\Breeze
- C:\ProgramData\MedGraphics\Breeze

**Note:** The C:\ProgramData folder is normally hidden.

All BreezeSuite users must have either a minimum of Full Control basic permissions or Query Value, Set Value and Create SubKey advanced permissions to the following registry and all child objects:

- x86 Operating Systems = H-Key-Local-Machine\Software\Medical Graphics Corporation\
- x64 Operating Systems = H-Key-Local-Machine\Software\Wow64\Medical Graphics Corporation\

## Special Windows User Permissions required on Ultima Carido2 systems running Mortara XScribe software:

All BreezeSuite users must have their Security User Permissions set to 'Full control' for the following folders and all child objects:

- C:\Program Files (x86)\Mortara
- C:\Mortara Instrument Inc
- C:\ProgramData\MedGraphics\XScribe\
- C:\ECG Data

All BreezeSuite users must have their Security User Permissions set to 'Full control' for the following folders and all child objects:

- C:\ProgramData\ExamMgrData

## Special Antivirus and anti-malware requirements on Ultima Cardio2 systems running Mortara XScribe software:

BreezeSuite and Mortara XScribe software communicate and store data in real-time during testing. The files exchanged in the following directories and/or files must be excluded from active scanning or software failure and data loss may occur.

- C:\ECG Data
  - File Names:
    - CFD.xml
    - CFDL.xml
    - CFV.xml
    - LinkEcg.xs2
    - LogFile.txt
    - ModalityPermissionsTable.xml
    - RawEcg.xs2

- Report\_Cardiopulmonary.xml
  - ST.cfg
  - Step.xs2
  - StressExamSettings.xml
  - StressExamSummary.xml
  - XSPrintOps.txt
- C:\ProgramData\MedGraphics\XScribe\Command  
File Names:
  - BreezeLog.txt
  - Mort.txt
  - ToBreeze.cmd
- C:\ProgramData\MedGraphics\XScribe\Current  
File Names:
  - CFD.xml
  - CFSL.xml
  - CFV.xml
  - LinkEcg.xs2
  - RawEcg.xs2
  - ModalityPermissionsTable.xml
  - Report\_Cardiopulmonary.xml

**File Compression must not be enabled on the following folder:**

- C:\Program Files (x86)\Microsoft SQL Server\MSSQL12.MGCSQLSERVER\MSSQL

**Verify and delete (if necessary) the MedGraphics Virtual Store directory.**

*Delete the Medical Graphics VirtualStore program folder*

1. Click on File Explorer, then select the View tab; checkmark the box by **Hidden Items**.
2. Click on the "**This PC**" shortcut, then double click on the following:
  - a. C:\Users\ValuedCustomer\AppData\Local\VirtualStore\ProgramFiles (x86)
3. Delete the MedGraphics folder..

*Delete the Medical Graphics VirtualStore registry entry.*

1. In the Windows desktop search box, type **regedit**.
2. Browse to HKEY USERS\... 'registry string'...\_Classes \VirtualStore\Machine\Software\WOW6432Node\Medical Graphics Corporation.  
**Note:** Only one of the \_Classes registry strings will have the VirtualStore folder.
3. Right Click on the Medical Graphics Corporation folder and click delete.
4. Close the registry editor window.

**Disable Virtual Stores:**

1. Open the Windows Control Panel.
2. Select Administrative Tools.
3. Select Local Security Policy.
4. Open Local Policies.
5. Open Security Options.
6. Scroll down and double click on User Account Control: Virtualize file and registry write failure to per-user locations.
7. Select 'Disabled' and click OK.

## Printer Setup:

For the PDF reports to work properly, the properties of PDF reports need to be updated to Adobe Acrobat Reader from Edge (Microsoft's browser within Windows 10). Edge does not have a File Explorer properties 'Print', so BreezeSuite cannot start a PDF print without this.

1. From the Windows start menu, type "Default Programs."
2. Select "Choose default apps by file type."
3. Scroll down to ".pdf" Adobe Acrobat Document.
4. Click "Choose a default."
5. Select Adobe Reader

In addition, take the checkmark out to let windows control the default printer; by default, it is checked and defaults to the Medgraphics PDF printer, which is suitable for exporting purposes only.

1. From the Windows start menu, type "Printers & Scanner."
2. Scroll down past printer options and uncheck "Let Windows manage my default printer."
3. Pick the appropriate printer for your organization.

# BREEZESUITE V8.6 STANDALONE CLIENT UPGRADE

**Important:** Upgrade of BreezeSuite requires Windows Administrator permission.

**Important:** Ensure your Windows Operating System is up-to-date with the latest updates and restart the computer to ensure there are no pending reboots.

**Important:** Upgrade to BreezeSuite v8.6 requires SQL Server Express 2014 SP3. . The upgrade to SQL Server 2014 Express SP3 is included with the BreezeSuite 8.6 software media and instructions are included in this manual.

## Upgrade Procedure:

### 1. Backup Local Patient Database


1.1. Select the Windows Start menu

1.1.1. Windows 7 users, Select 'All Programs > MedGraphics > DBTools'

1.1.2. Windows 10 users, Select 'Medgraphics > DBTools'

1.2. If prompted, enter the User Name and Password with Backup Database permissions into the DBTools login window and select 'OK'

1.3. Select the 'Tools > Backup Databases > Local Patient Database' menu item

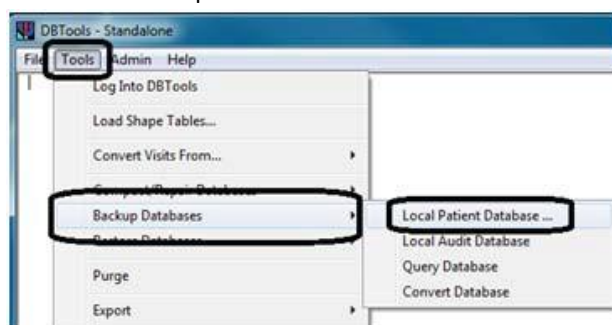


1.4. Select 'OK' when prompted with "A database must by default be backed up to the machine it is running on..." message

1.5. Enter the MGCAdmin SQL User password and press 'OK' to continue


**Note:** "Breeze2007" is the default password set during BreezeSuite installation

1.6. Select the "Backup To" location



1.7. Browse to the SQL Backup folder or other folder where you place your database backups


1.8. Select 'Open' to begin the Local Patient Database backup.

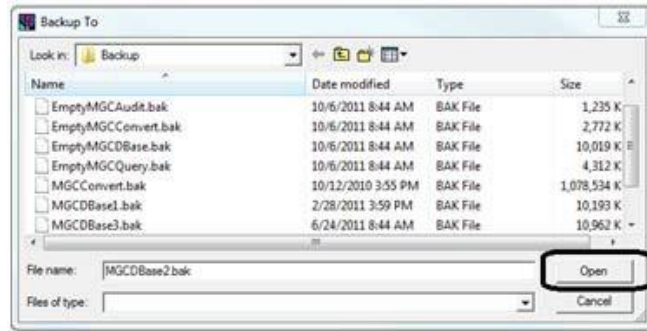


1.9. Wait for the "Backup Completed Successfully" message to appear and close DBTools.

## 2. Upgrade SQL Server Express instance to SQL Server Express 2014 SP3

2.1. Browse to the "Launch.exe" file located on your installation media (USB flash drive, etc.).




2.2. Right Click on the "Launch.exe" file and select 'Run as Administrator'

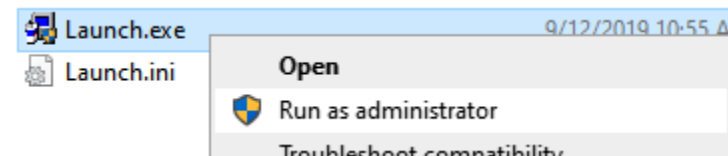


2.3. Select 'INSTALL SOFTWARE'




2.4. Select 'WORKSTATION'

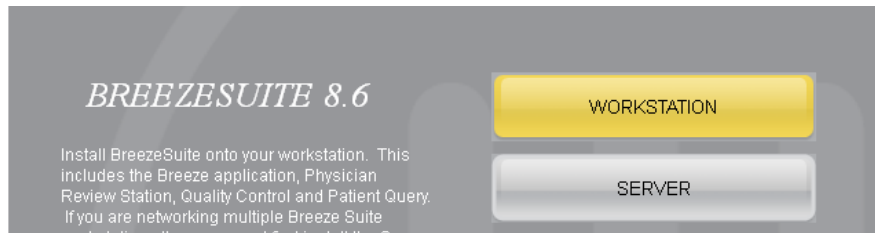

2.5. Select 'MICROSOFT SQL SERVER' button to start SQL Server upgrade

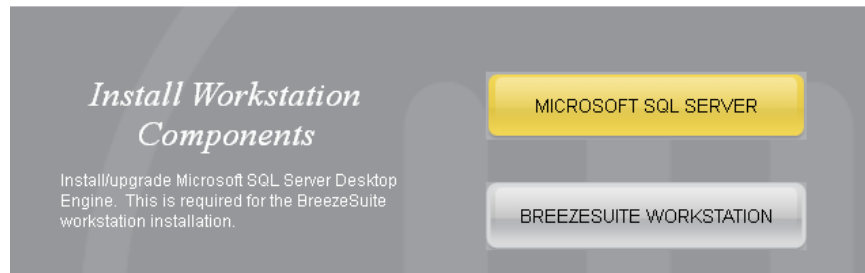


2.6. Select 'Yes' after you have verified you have created a backup of the BreezeSuite database

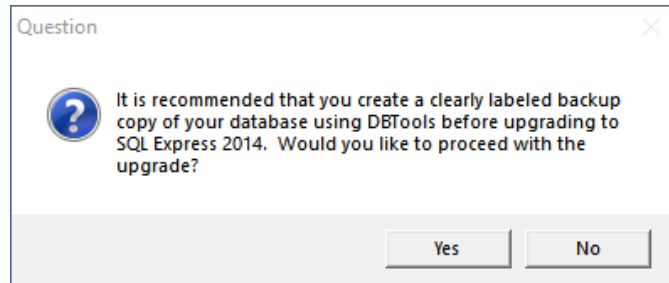


2.6.1. Desktop Engine Setup windows will appear and may remain open for several minutes. Please wait for the upgrade process to start.

2.6.2. When the SQL Server 2014 SP3 upgrade process starts, it may take several additional minutes to complete. Please wait for the upgrade process to complete.

2.7. If prompted, Enter the SA password for the SQL Server Express instance to be upgraded.


 **Note:** If default password was used on previous installation, password is set to "Breeze2007"

 **Important:** Use of a strong password longer than 12 characters, containing upper case alpha, lower case alpha, numeric and special characters is recommended. If Default password was used on previous installations, the SA password should be changed using Microsoft SQL Server Management Studio either prior to or after upgrade is complete.



2.8. Wait for the upgrade process to complete. This process may take several minutes

- 2.9. Select 'OK' when prompted with "Installation of SQL Server Express is complete" message.
- 2.9.1. If prompted with "setup requires that the system be rebooted" message. Select 'OK' and reboot.

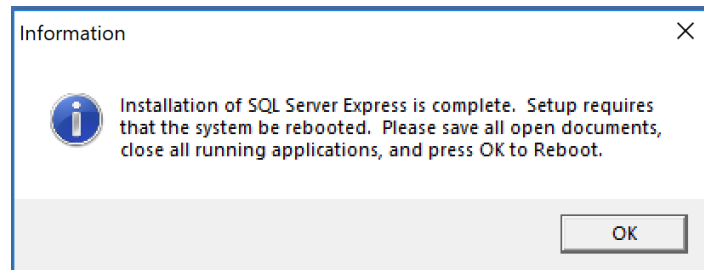


### 3. Upgrade BreezeSuite software to BreezeSuite v8.6


- 3.1. Select 'INSTALL SOFTWARE'



- 3.2. Select 'WORKSTATION'

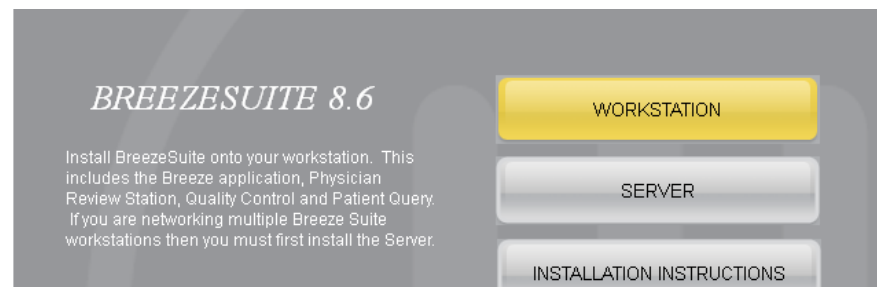


- 3.3. Select 'BREEZESUITE WORKSTATION' on the Install Workstation Components screen.

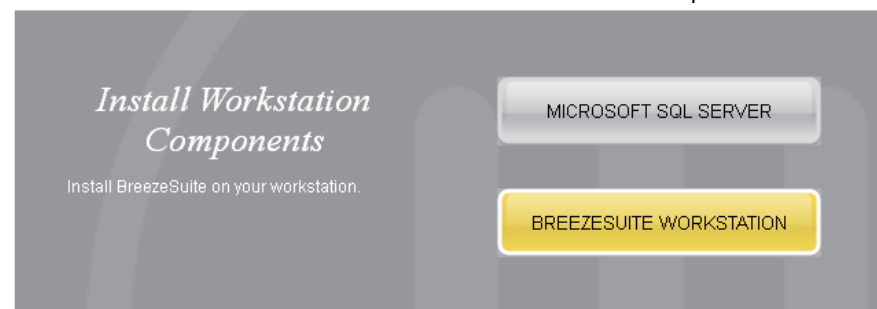


3.4. Select 'Next >' at the bottom of the "Welcome to the InstallShield Wizard..." screen

3.5. Read the License Agreement and select 'Yes' to accept the terms continue with the upgrade

 **Note:** A copy of the EULA is provided at the end of this document for review prior to software upgrade.


3.6. Verify you have created a backup of the BreezeSuite database and select 'OK' to proceed with upgrade.

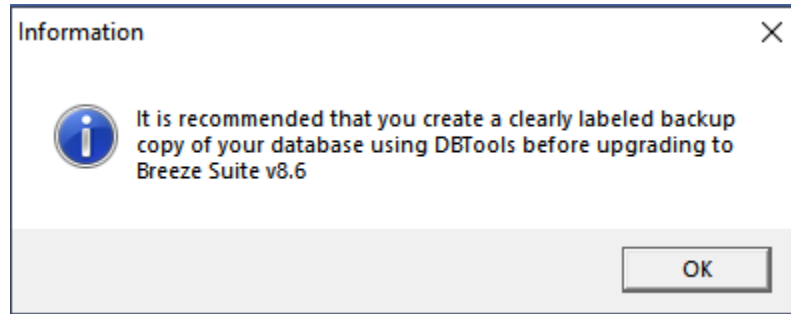

### 3.9 BreezeSuite 8.6 License Screen

- a. If upgrading from version 8.0 or higher, complete the Name and Company fields with any text data and select 'Next >'
- b. If upgrading from version 7.2, contact MGC Diagnostics support by calling 800-333-4137. Please have your account number, system serial number or sales order number and software registration number displayed on the licensing screen available.

Complete the Name and Company fields with any text data and enter the CD Key provided for the upgrade in the CD Key fields. Select 'Next >' to continue with the upgrade.

 **Note:** Customers outside the United States must contact their regional MGC Diagnostics distributor to obtain a software license (CD Key).

3.10 Review the upgrade settings within the "Start Copying Files" screen and select 'Next >'

3.11 Select 'Finish' on the "InstallShield Wizard Complete" screen.

# BREEZESUITE SOFTWARE LICENSE AGREEMENT

## BREEZE SUITE LICENSE AGREEMENT FOR MEDICAL GRAPHICS SOFTWARE

**IMPORTANT READ CAREFULLY:** This Medical Graphics Corporation License Agreement (Agreement) is a legal agreement between you (either an individual or a single entity) and Medical Graphics Corporation for the software product identified above, which includes computer software and associated media and printed materials, and may include online or electronic documentation (SOFTWARE PRODUCT or SOFTWARE). By installing, copying or otherwise using the SOFTWARE PRODUCT, you agree to be bound by the terms of this AGREEMENT. If you do not agree to the terms of this AGREEMENT, promptly return the unused SOFTWARE PRODUCT to the place from which you obtained it.

### Software PRODUCT LICENSE

The SOFTWARE PRODUCT is protected by copyright laws and international copyright treaties, as well as other intellectual property laws and treaties. The SOFTWARE PRODUCT is licensed, not sold.

#### 1. GRANT OF LICENSE. This AGREEMENT grants you the following rights:

**Systems Software.** You may install and use one copy of the SOFTWARE PRODUCT on a single computer. If the SOFTWARE PRODUCT includes functionality that enables your single computer to act as a network server, any number of computers or workstations may access or otherwise utilize the basic network services of that server. The basic network services are more fully described in the printed materials accompanying the SOFTWARE PRODUCT.

**Storage/Network Use.** You may also store or install a copy of the SOFTWARE PRODUCT on a storage device, such as a network server, used only to install or run the SOFTWARE PRODUCT on your other computers over an internal network; however, you must acquire and dedicate a license for each separate computer on which the SOFTWARE PRODUCT is installed or run from the storage device. A license for the SOFTWARE PRODUCT may not be shared or used concurrently on different computers.

#### 2. DESCRIPTION OF OTHER RIGHTS AND LIMITATIONS.

**Limitations on Reverse Engineering, Decompilation and Disassembly.** You may not reverse engineer, decompile, or disassemble the SOFTWARE PRODUCT, except and only to the extent that such activity is expressly permitted by applicable law notwithstanding this limitation.

**Separation of Components.** The SOFTWARE PRODUCT is licensed as a single product. Its component parts may not be separated for use on more than one computer.

**Single Machine.** The SOFTWARE PRODUCT may only be used with the single computer on which it was first installed.

**Rental.** You may not rent or lease the SOFTWARE PRODUCT.

**Systems Software Transfer.** You may permanently transfer all of your rights under this AGREEMENT only as part of a sale or transfer of your single computer system where the SOFTWARE PRODUCT is installed, provided you retain no copies, you transfer all of the SOFTWARE PRODUCT (including all component parts, the media and printed materials, any upgrades, this AGREEMENT and, if applicable, the Certificate of Authenticity), and the recipient agrees to the terms of this AGREEMENT. If the SOFTWARE PRODUCT is an upgrade, any transfer must include all prior versions of the SOFTWARE PRODUCT.

**Termination.** Without prejudice to any other rights, Medical Graphics may terminate this AGREEMENT if you fail to comply with the terms and conditions of this AGREEMENT. In such event, you must destroy all copies of the SOFTWARE PRODUCT and all of its component parts.

**3. UPGRADES.** If the SOFTWARE PRODUCT is an upgrade from another product, whether from Medical Graphics or another supplier, you may use or transfer the SOFTWARE PRODUCT only in conjunction with that upgraded product, unless you destroy the upgraded product. If the SOFTWARE PRODUCT is an upgrade of a Medical Graphics product, you now may use that upgraded product only in accordance with this AGREEMENT. If the SOFTWARE PRODUCT is an upgrade of a component of a package of software programs which you licensed as a single product, the SOFTWARE PRODUCT may be used and transferred only as part of that single product package and may not be separated for use on more than one computer.

4. **COPYRIGHT.** All title and copyrights in and to the SOFTWARE PRODUCT (including but not limited to any images, photographs, animations, video, audio, music, text and applets, incorporated into the SOFTWARE PRODUCT), the accompanying printed materials, and any copies of the SOFTWARE PRODUCT, are owned by Medical Graphics or its suppliers. The SOFTWARE PRODUCT is protected by copyright laws and international treaty provisions. Therefore, you must treat the SOFTWARE PRODUCT like any other copyrighted material except that you may either (a) make one copy of the SOFTWARE PRODUCT solely for backup or archival purposes, or (b) install the SOFTWARE PRODUCT on a single computer provided you keep the original solely for backup or archival purposes. You may not copy the printed materials accompanying the SOFTWARE PRODUCT.

5. **DUAL-MEDIA SOFTWARE.** You may receive the SOFTWARE PRODUCT in more than one medium. Regardless of the type or size of medium you receive, you may use only one medium that is appropriate for your single computer. You may not use or install the other medium on another computer. You may not loan, rent, lease, or otherwise transfer the other medium to another user, except as part of the permanent transfer (as provided above) of the SOFTWARE PRODUCT.

6. **U.S. GOVERNMENT RESTRICTED RIGHTS.** The SOFTWARE PRODUCT and documentation are provided with RESTRICTED RIGHTS. Use, duplication, or disclosure by the Government is subject to restrictions as set forth in subparagraph (c)(1)(ii) of the Rights in Technical Data and Computer Software clause at DFARS 252.227-7013 or subparagraphs (c)(1) and (2) of the Commercial Computer Software Restricted Rights at 48 CFR 52.227-19, as applicable. Manufacturer is Medical Graphics Corporation, St. Paul, Minnesota.

#### MISCELLANEOUS

If you acquired this product in the United States, this AGREEMENT is governed by the laws of the State of Minnesota.

If this product was acquired outside the United States, then local law may apply.

Should you have any questions concerning this AGREEMENT, or if you desire to contact Medical Graphics for any reason, please write: Medical Graphics, 350 Oak Grove Parkway, St. Paul, Minnesota, 55127; or [www.Medgraph.com](http://www.Medgraph.com), or contact the Medical Graphics distributor serving your country.

#### LIMITED WARRANTY

**LIMITED WARRANTY.** Medical Graphics warrants that the SOFTWARE PRODUCT will perform substantially in accordance with the accompanying written materials for a period of ninety (90) days from the date of receipt. Some states and jurisdictions do not allow limitations on duration of an implied warranty, so the above limitation may not apply to you. To the extent allowed by applicable law, implied warranties on the SOFTWARE PRODUCT and hardware, if any, are limited to ninety (90) days and one year, respectively.

**CUSTOMER REMEDIES.** Medical Graphics's and its distributors' entire liability and your exclusive remedy shall be, at Medical Graphics's option, either (a) return of the price paid, or (b) repair or replacement of the SOFTWARE PRODUCT that does not meet Medical Graphics's Limited Warranty and which is returned to Medical Graphics. This Limited Warranty is void if failure of the SOFTWARE PRODUCT has resulted from accident, abuse, or misapplication. Any replacement SOFTWARE PRODUCT will be warranted for the remainder of the original warranty period or thirty (30) days, whichever is longer. Outside the United States, neither these remedies nor any product support services offered by Medical Graphics are available without proof of purchase from an authorized international source.

**NO OTHER WARRANTIES.** TO THE MAXIMUM EXTENT PERMITTED BY APPLICABLE LAW, MEDICAL GRAPHICS AND ITS SUPPLIERS DISCLAIM ALL OTHER WARRANTIES, EITHER EXPRESS OR IMPLIED, INCLUDING, BUT NOT LIMITED TO, IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE, WITH REGARD TO THE SOFTWARE PRODUCT, AND ANY ACCOMPANYING HARDWARE. THIS LIMITED WARRANTY GIVES YOU SPECIFIC LEGAL RIGHTS. YOU MAY HAVE OTHERS, WHICH VARY FROM STATE/JURISDICTION TO STATE/JURISDICTION. **NO LIABILITY FOR CONSEQUENTIAL DAMAGES.** TO THE MAXIMUM EXTENT PERMITTED BY APPLICABLE LAW, IN NO EVENT SHALL MEDICAL GRAPHICS OR ITS SUPPLIERS BE LIABLE FOR ANY SPECIAL, INCIDENTAL, INDIRECT OR CONSEQUENTIAL DAMAGES WHATSOEVER (INCLUDING, WITHOUT LIMITATION, DAMAGES FOR LOSS OF BUSINESS PROFITS, BUSINESS INTERRUPTION, LOSS OF BUSINESS INFORMATION, OR ANY OTHER PECUNIARY LOSS) ARISING OUT OF THE USE OF OR INABILITY TO USE THE SOFTWARE PRODUCT, EVEN IF MEDICAL GRAPHICS HAS BEEN ADVISED OF THE POSSIBILITY OF SUCH DAMAGES. BECAUSE SOME STATES AND JURISDICTIONS DO NOT ALLOW THE EXCLUSION OR LIMITATION OF LIABILITY FOR CONSEQUENTIAL OR INCIDENTAL DAMAGES, THE ABOVE LIMITATION MAY NOT APPLY TO YOU.

MGC DIAGNOSTICS CORPORATION, through its subsidiary Medical Graphics Corporation  
350 Oak Grove Parkway St. Paul, Minnesota USA 55127-8599

© 2022 MGC Diagnostics Corporation or one of its affiliates. All rights reserved.

All specifications subject to change without notice. Products may vary from those illustrated.

MGC Diagnostics and its affiliates are equal opportunity/affirmative action employers committed to cultural diversity in the workforce.

Part# 142233-001 RevA