

# Six Minute Walk Test

with Ascent™ cardiorespiratory diagnostic software



Testing patients was just made easier by combining Ascent™ software's six-minute walk test (6MWT) option with the Nonin® WristOx<sub>2</sub>™ 3150 Bluetooth Pulse Oximeter. Since testing is being performed within Ascent™ cardiorespiratory diagnostic software, there is no need for long cables or transferring of data from one device to another. The pulse oximeter data is captured seamlessly within Ascent software and is stored directly to the software's database.




NONIN® WRISTOX<sub>2</sub>™ 3150  
PULSE OXIMETER  
with finger sensor

## BENEFITS

- **Mobile Solution:** designed for touchscreen functionality, the integrated Bluetooth® capability means you no longer need to walk side-by-side with the patient in order to read the heart rate and saturation from the pulse oximeter.
- **Additional Data:** such as Dyspnea and Leg Fatigue scores, can be added on-the-move with simple icons and drop-down menus. Supplemental information for walking device, oxygen device and liter flow are available at the touch of a finger.
- **Flexibility:** with the ability to add or change the oxygen device and liter flow mid-test, the 6MWT software can also be used for O<sub>2</sub> Titration testing. The software also allows you to set the test time for greater than six minutes, allowing you to observe the patient through different phases of room air and oxygen concentrations.



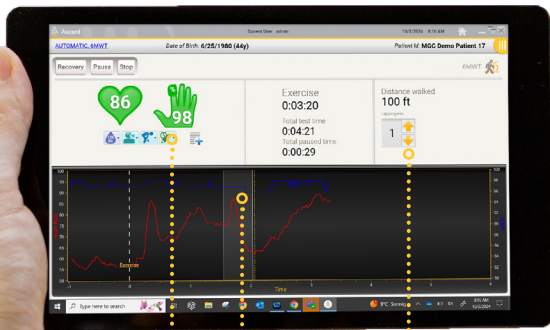


Touch Screen Icons

Graphic Display of Pause(s)

One-Touch Lap Increase

## DATA DISPLAY AND REPORTS

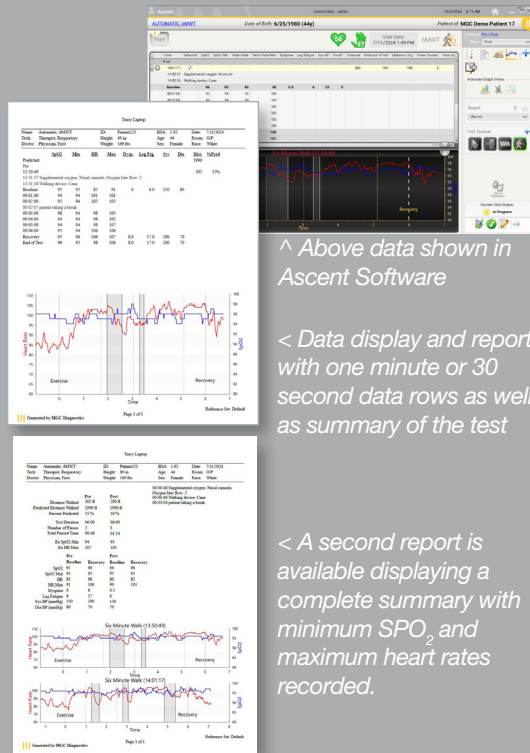

## CHOOSE YOUR TESTING OPTION

The Nonin® WristOx<sub>2</sub>™ allows you to choose the sensor technology that is right for your patient and facility. Both options send data directly into Ascent Software for continuous real-time display of data.



### FINGER SENSOR

Reusable soft sensor available in three sizes from children to adult.




### FOREHEAD SENSOR

Optimal for patients with mobility challenges who need their hands free for walking support.

## REAL-TIME PROMPTS

Real-time prompts, which follow the ATS/ERS Technical Standard, are displayed to allow you to have standardized encouragement during testing.



## SPECIFICATIONS

### COMPUTER

- Microsoft Windows® based (10 or 11) laptop or tablet running Ascent software
- Bluetooth® capabilities (version 2.0 or higher)

### PULSE OXIMETER

- Nonin® WristOx<sub>2</sub>™ Model 3150 classic (non BLE)
- SpO<sub>2</sub>: 0% to 100%
- Pulse Rate Range: 18-321BPM
- Sensors: Finger, Reflectance
- Battery: Two 1.5v AAA

MGC DIAGNOSTICS CORPORATION, through its subsidiary Medical Graphics Corporation  
350 Oak Grove Parkway St. Paul, Minnesota USA 55127-8599

© 2024 MGC Diagnostics Corporation or one of its affiliates. All rights reserved.  
All specifications subject to change without notice. Products may vary from those illustrated.  
MGC Diagnostics and its affiliates are equal opportunity/affirmative action employers committed to cultural diversity in the workforce.

Part# 061385-001 RevA

CE 2797

